



Triglyceride Assay Kit-Bulk 500 Point Assay Kit, 96 well format Cat# TG-5-RB

INSTRUCTION MANUAL ZBM0014.07

STORAGE CONDITIONS

- **Reagents A & Buffers:**

Store at 2 - 8°C. **Use reconstituted Glycerol Reagent A within 7 days.**

- **Glycerol Standard & Reagent B**

-20°C **NEW REAGENT B STORAGE TEMPERATURE**

ALL ZEN-BIO INC PRODUCTS ARE FOR RESEARCH USE ONLY. NOT APPROVED FOR HUMAN OR VETERINARY USE OR FOR USE IN DIAGNOSTIC OR CLINICAL PROCEDURES.

LIMITED PRODUCT WARRANTY

This warranty limits our liability to replacement of this product. No other warranties of any kind, expressed or implied, including without limitation, implied warranties of merchantability or fitness for a particular purpose, are provided by Zen-Bio, Inc. Zen-Bio, Inc. shall have no liability for any direct, indirect, consequential, or incidental damages arising out of the use, the results of use, or the inability to use this product.

ORDERING INFORMATION AND TECHNICAL SERVICES

- **Zen-Bio, Inc.**
- **3920 South Alston Avenue**
- **Durham, NC 27713**
- **Telephone** (919) 547-0692
- **Facsimile (FAX)** (919) 547-0693
- **Toll Free** 1-866-ADIPOSE (866)-234-7673
- **Electronic mail (e-mail)** information@zen-bio.com
- **World Wide Web** <http://www.zenbio.com>

The contents of this kit are sufficient for the assay of up to five 96 well plates (500 assay points). The protocol is designed for assay of cells in a 96-well format. For other formats, please adjust the volumes added to each well according to the surface area of the well/flask you are using. See your cultureware manufacturer's technical information for the specifications.

ITEMS INCLUDED IN THE KIT

Item	Instructions	Amount	QTY	Storage
Wash Buffer		250 ml	1	4°C
Lysis Buffer		15 ml	1	4°C
Reagent A	Reconstitute w/ 40 ml deionized water. Reconstitute w/ 11 ml deionized water. Combine and mix before use. Use reconstituted Reagent within 7 days.	40ml 11ml	1 1	4°C
Reagent B	11 ml Reagent B solution. New storage temperature	11ml	1	-20°C
Glycerol standard	Glycerol @ 1mM [Reconstitute with 400 µl Standards Diluent to make the 200 µM glycerol standard; see manual for recommended dilution scheme]	100 µl	3	-20°C
Standards Diluent		11 ml	1	4°C


Other equipment/reagents required but not provided with the kit:

- ▶ Single-channel pipetter
- ▶ Multi-channel pipetter
- ▶ Plate reader with a filter of 540 nm
- ▶ Tubes to dilute glycerol standards
- ▶ Disposable reagent trays
- ▶ Mature adipocytes or other cells
- ▶ Clear bottom 96-well assay plates

ASSAY PROCEDURE

1. Warm the Wash buffer and Lysis buffer in a 37°C water bath.
2. Thaw Reagent B solution to Room Temperature and gently invert. DO NOT VORTEX! Store in a light protected bottle. Reagent B may be refrozen and stored (-20°C). Avoid repeated freeze/thaw cycles.
3. Remove all media from mature human adipocytes. Using about 15 ml of the wash buffer, wash the cells one time with 150 µl wash buffer. Label the disposable tray “wash buffer” and retain for later use.
4. Remove all Wash buffer. Using a disposable reagent tray (not provided), add 15 µl Lysis buffer per well. Incubate at 37°C - 50°C for 20 minutes.
5. After the incubation is complete, visually confirm cell lysis by checking the wells under a microscope. If cells are not fully lysed, incubate for another 10 minutes. Sometimes pipet mixing is necessary for full lysis.
6. Add 135 µl warm Wash Buffer to each well.
7. Add 20 µl Reagent B to each well. It is not necessary to mix at this time, however, gently tap plate to help mix reagents. Incubate the plate at 37°C for 2 hours.
8. One hour prior to the assay, bring the glycerol standard and Reagent A to room temperature. Warm the Standards Diluent to 37°C. Prepare the standard curve as follows:

Pipette 400 µl of the Standards Diluent into the 1 mM glycerol standard tube provided and mix well by vortexing. This produces a diluted stock glycerol standard of 200 µM. Pipette 250 µl of Diluent into 6 tubes (not provided). Using the newly diluted stock glycerol solution, prepare a dilution series as depicted below. Mix each new dilution thoroughly before proceeding to the next. The 200 µM stock dilution serves as the highest standard; the Diluent serves as the zero standard.

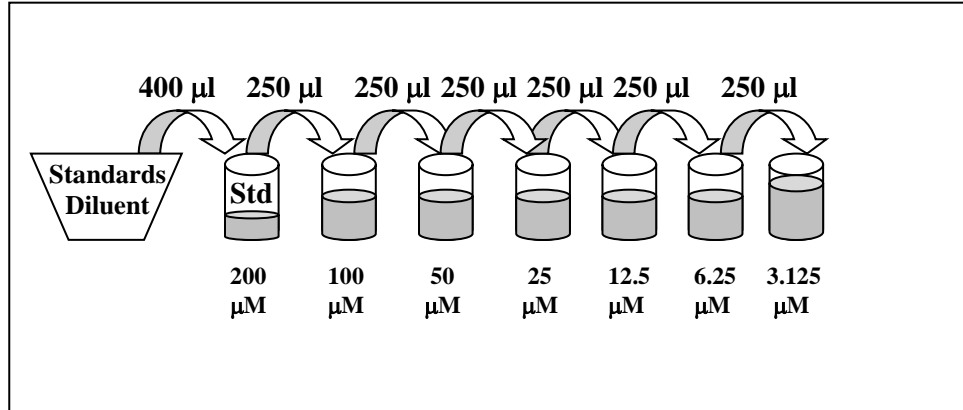

Note: The above dilution series generates enough volume to perform the standard curve in duplicate. If you wish to perform the standard curve in duplicate, please note that eight fewer data points can be assayed with this kit.

9. Also at this time prepare the Reagent A by adding 40 ml and 11 ml respectively of deionized water to the appropriate bottle and gently invert. DO NOT VORTEX! Use a pipet to ensure that the powder is completely dissolved. Mix and combine the 2 volumes for use in the assay. Keep at room temperature. If using a Glycerol Reagent A solution previously prepared and stored at 2-8°C, also bring to room temperature. Make sure there is enough Glycerol Reagent A from one solution to treat all the points in the assay. It may be necessary to combine solutions. Store in a light protected bottle. Reconstituted Glycerol Reagent A is stable for 7 days refrigerated (2-8°C); store any remaining solution refrigerated (2-8°C).
10. To a blank 96 well plate (not provided), add 80 μl Wash Buffer to each well needed for the assay (NOTE: do not add Wash Buffer to the wells used for the standard curve).
11. Working with one row or column at a time, mix the lysates very well using a multi-channel pipet. Immediately transfer 20 μl per well of the lysates to the corresponding well of the plate containing the wash buffer. **This results in a Dilution Factor of 5.**
12. Prepare the standard curve. Pipet 100 μl of each standard into a well. (NOTE: Eight wells are necessary for the curve. If there are remaining wells on the assay plate, you can utilize the remaining wells.)
13. Add 100 μl Reagent A to samples and standards. Mix by pipetting up and down one time. Incubate at room temperature for 15 minutes.
14. Read at 540 nm using a microtiter plate reader.

GLYCEROL STANDARD CURVE

This kit is designed to show relative lipid accumulation of experimental treatments compared to controls. The assay is based on the equation



The reagent measures the concentration of glycerol released after lysing the cells and hydrolyzing the triglyceride molecules. The triglyceride concentration can then be determined from the glycerol values.


Generate standard curve: see example below

[DO NOT use this standard curve to generate your data. This is an example.]

- Subtract the OD value of the 0 μ M standard from all OD values including the standard curve.

Glycerol (uM)	OD	OD	OD-blank	OD-blank	Avg OD-blank
0	0.048	0.048			0.048
3.125	0.059	0.058	0.011	0.01	0.059
6.25	0.07	0.07	0.022	0.022	0.070
12.5	0.098	0.098	0.05	0.05	0.098
25	0.127	0.13	0.079	0.082	0.129
50	0.2	0.205	0.152	0.157	0.203
100	0.353	0.362	0.305	0.314	0.358
200	0.649	0.667	0.601	0.619	0.658

slope	0.003
intercept	0.053
R ²	0.9997

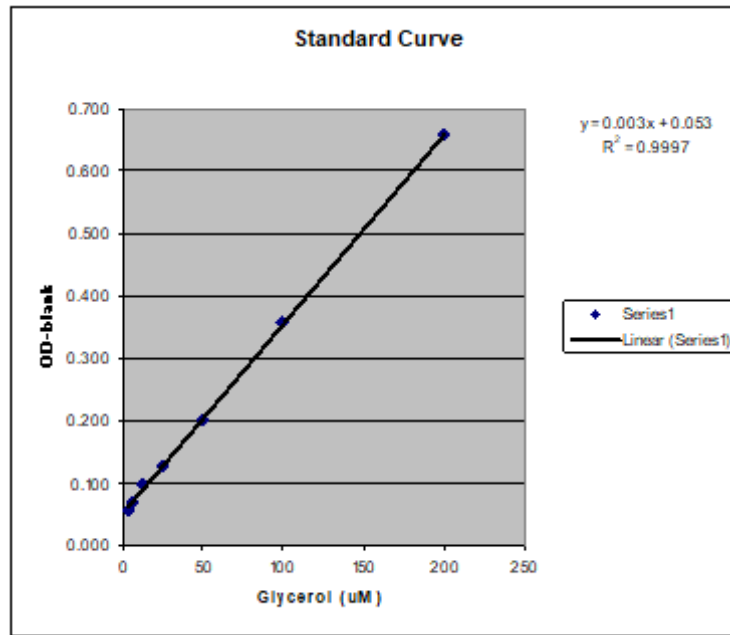

y = observed O.D. minus the blank

x = concentration of glycerol in μM

To calculate x for each y , (i.e. to change the observed O.D. into glycerol concentration) use the following equation:

$y = (\text{slope}) \times (x) + \text{intercept}$

$y = mx + b$ so $x = (y - b) / m$

$x = (y - 0.0006) / 0.0014$ where $0.0014 =$ slope of the line and $0.0006 =$ y intercept.

Be careful to enter the proper sign for the y intercept value as it may be a negative number.

Any OD values greater than the highest standard ($200 \mu\text{M}$) should be suspect. The compound should be re-assayed using a lower dose of the compound at treatment OR a dilute solution of the condition medium at the time of the assay.

The R^2 value should be equal or greater then 0.98 for the standard curve to be valid. Any R^2 values below 0.98, must have the standard curve run again.

Solve for the Total Glycerol concentration (i.e. total triglyceride concentration) for each OD. **Remember to include the Dilution Factor in the equation.**

Data is expressed as μM Glycerol.

NOTE: Any OD values that are negative after the blank is subtracted should be considered to be 0 for the OD value.

FREQUENTLY ASKED QUESTIONS

1. **Can I buy the reagents separately?** The only reagents sold separately are Glycerol Reagent A (cat# RGTA-10; RGTA-40) and the glycerol standard for the Triglyceride Assay kit (cat# TG-GLYSTAN).
2. **Can I use another plate format besides 96 well?** This kit is designed for the assay of A 96 well plate (100 assay points). We do not have a protocol for other formats.
3. **Can I use this kit to measure total triglyceride in other cell lines and other human and non-human cells?** Yes. The assay is not species specific. As long as the sample concentration is in the linear range, this kit should be able to detect it.
4. **My cells did not lyse.** What can I do? If cells are not fully lysed, incubate for another 10 minutes at 37°C - 50°C. Sometimes mixing by pipetting up and down several times is necessary for full lysis.
5. **I do not have time to complete the assay. Can I freeze the samples?** Yes. The cell lysates can be stored at -80°C for a maximum of 7 days. Mix the thawed lysates in the plate by pipetting up and down several times. Allow all reagents and samples to reach room temperature BEFORE adding the Wash Buffer and Glycerol Reagent A to complete the assay.

TROUBLESHOOTING

Problem	Suggestions
High background or the triglyceride reagent turns a darker color before the assay begins.	<ul style="list-style-type: none"> • Use clean tray and tips • Change pipet tips frequently
Edge effects	<ul style="list-style-type: none"> • Ensure a saturated humidity in the incubator to prevent evaporation from the outside wells
Inconsistent OD reading	<ul style="list-style-type: none"> • Be careful when pipetting to avoid bubbles. If bubbles persist, burst the bubbles using a large gauge needle prior to reading and read the plate again.

- Mix the lysates well before transferring the 20µl to the Wash buffer plate.

REFERENCES

1. Green, H. and Kehinde, O. (1974) Sublines of mouse 3T3 cells that accumulate lipid. *Cell* 1, 113-116.
2. Hauner, H., et al., (1989) *J. Clin. Invest.*(84), 1663-1670.
3. Kuri-Harcuch W, Wise LS, Green H. (1978) Interruption of the adipose conversion of 3T3 cells by biotin deficiency: differentiation without triglyceride accumulation. *Cell* 14:53-58.

APPENDIX A: PLATE LAYOUT

H	G	F	E	D	C	B	A	
								1
								2
								3

								4
								5
								6
								7
								8
								9
								10
								11
								12

APPENDIX B: TRIGLYCERIDE ASSAY FLOWCHART

