



# Human Adipocyte Lipolysis Assay Kit

## CAT# LIP-1-SPF

**INSTRUCTION MANUAL ZBM0049.01**

### **STORAGE CONDITIONS**

---

- 1 vial subcutaneous human preadipocytes,  $2.0 \times 10^6$  cells/vial: liquid nitrogen (LIP-1-SPF)
- Glycerol Reagent A, media & Buffers: 4°C
- Glycerol Standard & Controls: -20°C

***All Zen-Bio Inc products are for research use only. Not approved for human or veterinary use or for use in diagnostic or clinical procedures.***

### **LIMITED PRODUCT WARRANTY**

This warranty limits our liability to replacement of this product. No other warranties of any kind, expressed or implied, including without limitation, implied warranties of merchantability or fitness for a particular purpose, are provided by Zen-Bio, Inc. Zen-Bio, Inc. shall have no liability for any direct, indirect, consequential, or incidental damages arising out of the use, the results of use, or the inability to use this product.

### **ORDERING INFORMATION AND TECHNICAL SERVICES**


- Zen-Bio, Inc.
- 3200 Chapel Hill-Nelson Blvd., Suite 104
- PO Box 13888
- Research Triangle Park, NC 27709
- Telephone (919) 547-0692
- Facsimile (FAX) (919) 547-0693
- Toll Free 1-866-ADIPOSE (866)-234-7673
- Electronic mail (e-mail) [information@zen-bio.com](mailto:information@zen-bio.com)
- World Wide Web <http://www.zen-bio.com>

# INTRODUCTION

Lipolysis plays a central role in the regulation of energy balance. Lipolysis is the process in which triglycerides (TG) are hydrolyzed into glycerol and free fatty acids. This process releases free fatty acids (FFA) into the bloodstream where they may be either re-esterified by the adipocyte or travel to other tissues and exert other effects throughout the body. Elevated adipocyte lipolysis has been observed in obese and diabetic individuals (Arner 1996). Excessive free fatty acid production is believed to contribute to insulin resistance in skeletal muscle that is observed in obesity. Hormone sensitive lipase is the rate-limiting enzyme catalyzing triglyceride breakdown. Perilipins, one of the PAT (perilipins, adipophilin, IIP47 proteins) family of lipid-associated proteins, are implicated in adipocyte lipolysis by mediating the interaction of HSL with the triacylglycerol molecule (Brasaemle *et al.* 2004; reviewed in, Tansey *et al.* 2004.) The presence of these proteins corresponds to lipolytic stimulation in cultured adipocytes (Braemle *et al.* 2004).

The sympathetic nervous system also plays a key role in the regulation of lipid mobilization. The main lipolytic pathway involves beta-agonists ( $\beta$ -agonists), which activate  $\beta$ -adrenergic receptors via the intracellular  $G_s$  proteins in adipocytes. This leads to the activation of adenylate cyclase (AC), which then increases cyclic AMP (cAMP) levels. Elevated cAMP acts as a second messenger to activate hormone sensitive lipase (HSL). HSL, the rate-limiting enzyme regulating adipocyte lipolysis, then catalyzes the hydrolysis of triglycerides and results in the release of glycerol and FFA (increased lipolysis). Phosphodiesterases (PDE) are enzymes that hydrolyze cAMP to 5'-AMP (5 prime adenosine monophosphate). This action results in a decrease in lipolysis. PDE inhibitors increase intracellular cAMP levels. 3-isobutyl-1-methylxanthine (IBMX), a non-specific inhibitor of cAMP phosphodiesterases (PDE), is used as the positive control if your test compounds are suspected PDE inhibitors. Isoproterenol, a non-specific  $\beta$ -adrenergic agonist is used as the positive control if your test compounds affect lipolysis via  $\beta$ -adrenergic receptors (Robidoux *et al.* 2004).

This lipolysis assay kit provides the tool to study chemical compounds that may influence lipolysis in cultured adipocytes.

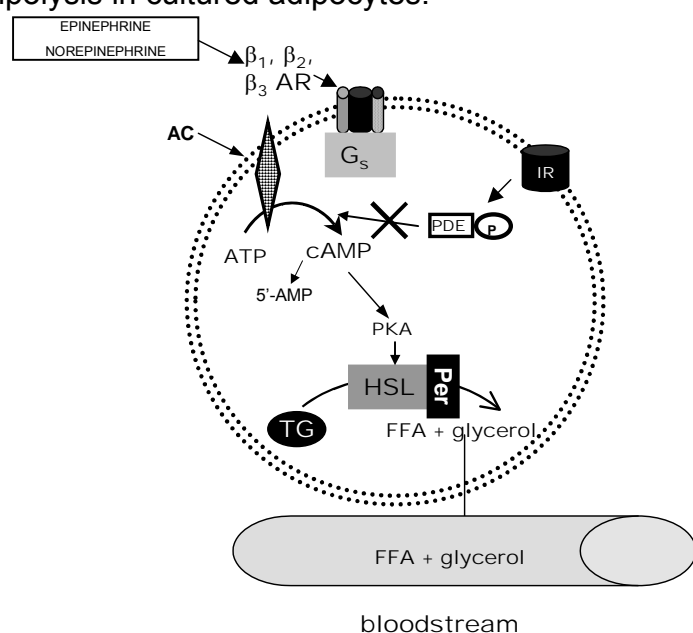



## ABBREVIATIONS:

AC	adenylate cyclase
AMP	adenosine monophosphate
AR	adrenergic receptors
ATP	adenosine triphosphate
$G_s$	G protein coupled receptor
IR	insulin receptor
FFA	free fatty acids
PDE	phosphodiesterase
PKA	protein kinase
Per	perilipins
TG	triglyceride
AMP	adenosine monophosphate
ATP	adenosine triphosphate
IR	insulin receptor
PDE	phosphodiesterase
Per	perilipins

**Figure 1. Overview of adipocyte lipolysis**

## PRINCIPLE OF THE ASSAY

Lipolytic activity is assessed by the measurement of glycerol released into the medium from triglyceride breakdown. Glycerol released to the medium is phosphorylated by adenosine triphosphate (ATP) forming glycerol-1-phosphate (G-1-P) and adenosine-5'-diphosphate (ADP) in the reaction catalyzed by glycerol kinase. G-1-P is then oxidized by glycerol phosphate oxidase to dihydroxyacetone phosphate (DAP) and hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>). A quinoneimine dye is produced by the peroxidase catalyzed coupling of 4-aminoantipyrine (4-AAP) and sodium N-ethyl-N-(3-sulfopropyl)m-anisidine (ESPA) with H<sub>2</sub>O<sub>2</sub>, which shows an absorbance maximum at 540nm. The increase in absorbance at 540nm is directly proportional to glycerol concentration of the sample.



## ITEMS INCLUDED IN THE KIT : LIP-1-SPF

ITEM	DESCRIPTION	Cap Color	UNIT	QTY	STORAGE
Cells	Cryopreserved human subcutaneous preadipocytes, 2.0X10 <sup>6</sup> cells/vial	---	VIAL	1	Liquid nitrogen
Blank Plates	Blank 96 well format plates for plating and/or assay	---	EACH	3	Room temp
Preadipocyte Medium	Preadipocyte Medium, 50.0 ml	CLEAR	BOTTLE	1	4°C
Differentiation Medium	Adipocyte Differentiation Medium, 25.0 ml	CLEAR	BOTTLE	1	4°C
Adipocyte Medium	Adipocyte Maintenance Medium, 25.0 ml	CLEAR	BOTTLE	1	4°C
LIP1 Assay Buffer	100 ml	---	BOTTLE	1	4°C
Wash Buffer	50 ml	---	BOTTLE	1	4°C
Vehicle	0.1% DMSO in LIP1 Assay Buffer	GREEN	1 ml / VIAL	1	-20°C
Positive Control	Isoproterenol, 10 mM in DMSO. <u>Dilute to 1 µM in Assay Buffer before use!</u> (i.e. 1 µl in 10 ml Assay Buffer)	BLUE	10 µl / VIAL	1	-20°C
Alternate Positive Control	3-Isobutyl-1-methylxanthine (IBMX), 100 mM in DMSO. <u>Dilute to 100 µM in Assay Buffer before use!</u> (i.e. 1 µl in 1 ml Assay Buffer)	RED	10 µl / VIAL	1	-20°C
Glycerol Reagent A (cat# RGTA-10)	Reconstitute with 11.0 ml deionized water prior to use.	BLACK	BOTTLE	1	4°C
Tray, non-sterile	For multi-channel pipetters, clear, non-sterile	---	EACH	2	----
Glycerol standard	Glycerol @ 1mM [Reconstitute with 400 µl Wash Buffer to make the 200 µM glycerol standard; see page 6 for recommended dilution scheme]	ORANGE	100 µl / VIAL	1	-20°C

### Other equipment/reagents required but not provided with the kit:

- Multi-channel pipet , single channel pipet and pipet tips; Tubes for diluting glycerol standards
- Sterile trays for multi-channel pipetters during plating & differentiation of cells
- Plate reader with a filter of 540 nm
- Incubator at 37°C
- Large gauge needle
- Option – Step 5 of Assay Procedure: 96 well plate, blank

## NOTE:

**THIS KIT IS DESIGNED FOR THE ASSAY OF A 96 WELL PLATE (100 ASSAY POINTS). YOU MAY USE THIS KIT TO ASSAY A SINGLE 384-, 96-, 24-, OR 12-WELL PLATE OF HUMAN ADIPOCYTES. YOU MUST THEN TRANSFER THE CONDITIONED ASSAY BUFFER TO A 96 WELL FORMAT TO COMPLETE THE ASSAY.**

## A. DIFFERENTIATION PROCEDURE

Please note: Primary cells can be very sensitive to brands of cultureware. Zen-Bio does not currently recommend the use of Falcon brand plates or flasks. Our scientists are using Nunc, Costar/Corning, or Greiner bio-one Cellstar tissue culture treated plates and flasks. Please contact us if you have any questions.

1. Remove cells from liquid nitrogen and place immediately into a 37° C water bath and agitate while in bath. Be careful not to submerge the cap of the vial into water. Do not leave the vials in water bath after most of the content has thawed. Rinse the vials with 70% ethanol before taking them to the culture hood.
2. Upon thawing, transfer the cells to a sterile conical bottom centrifuge tube containing 10 ml of Preadipocyte Medium (cat # PM-1). Centrifuge: 1,200 rpm (282 X g) / 20°C / 5 minutes. Aspirate the supernatant. TAKE CARE TO NOT ASPIRATE ANY OF THE CELL PELLET.
3. The cell vial contains a minimum of  $2.0 \times 10^6$  viable cells; however, we recommend performing a cell count to determine a more exact number of cells. Resuspend the cell pellet in 2 ml Preadipocyte Medium; dilute an aliquot in 0.4% trypan blue solution. We suggest withdrawing an aliquot of 50  $\mu$ l of cells and mixing with 100  $\mu$ l of the trypan blue solution, resulting in a dilution factor of 3. Count live (unstained) cells on a hemacytometer.
4. Plate approximately 40,625 cells /  $\text{cm}^2$  using the media volumes from the table below. Refer to the manufacturer's specifications for the specific cultureware brand you are using. See example below.

**Table 1. Plating Guide**

Brand	Plate Format	$\text{Cm}^2$ per well	Cells per $\text{cm}^2$	Cells per well	Total # Cells per plate	Total # cells for plating	Volume media per well	Total volume for plating
Costar	384	0.06	40,625	2,275	873,600	$9.1 \times 10^5$	30 $\mu$ l	12.0 ml
Costar	96	0.32	40,625	13,000	1,248,000	$1.3 \times 10^6$	150 $\mu$ l	15.0 ml
Greiner	48	1.02	40,625	41,438	1,989,000	$2.1 \times 10^6$	500 $\mu$ l	25.0 ml
Greiner	24	1.94	40,625	78,813	1,891,500	$2.0 \times 10^6$	1 ml	25.0 ml
Greiner	12	3.87	40,625	157,219	1,886,625	$2.0 \times 10^6$	2 ml	25.0 ml

**\*We recommend preparing slightly larger volumes to allow for loss due to foam and pipet error.**

5. Plate cells in desired format and place in a humidified 37°C incubator with 5%  $\text{CO}_2$ . Do not agitate the plate, as cells will not plate evenly.

6. Twenty-four hours after plating, check the plates for confluence. If they are not completely confluent, leave for an additional 24 hours maximum before inducing differentiation. If the cells are not confluent after 48 hours, DO NOT INDUCE DIFFERENTIATION (differentiation will be poor). Contact Zen-Bio immediately.
7. To start the differentiation process, aspirate the entire volume of Preadipocyte Medium from all wells. Add the appropriate volume of Adipocyte Differentiation Medium (catalog # DM-2) to the wells (see Table 1. Feeding Volumes). Incubate plate for 7 days at 37°C and 5% CO<sub>2</sub>.
8. After 7 days, cells should be fed by removing some of the media and replacing with fresh Adipocyte Medium (catalog # AM-1) (See Table 2. Feeding Volumes). **Caution: Do not dry the wells. Add new medium gently. If using an automatic feeder, set the slowest flow rate possible.**
9. Two (2) weeks after the initiation of differentiation, cells should appear rounded with large lipid droplets apparent in the cytoplasm. Cells are now considered mature adipocytes and are suitable for the lipolysis assay.

**Table 2. Feeding Volumes**

FORMAT	PLATING	CHANGE PM-1 TO DM-2		CHANGE DM-2 TO AM-1	
PLATE	IN	OUT	IN	OUT	IN
384 well	30 µl/well	30 µl/well	30 µl/well	18µl/well	24 µl/well
96 well	150 µl/ well	150 µl/ well	150µl/ well	90 µl/ well	120µl/ well
48 well	500 µl/ well	500µl/ well	500µl/ well	300µl/ well	40 µl/ well
24 well	1.0 ml/well	1.0 ml/well	1.0 ml/well	0.6 ml/well	0.8 ml/well
12 well	2.0 ml/well	2.0 ml/well	2.0 ml/well	1.2 ml/well	1.6 ml/well

**THIS KIT IS DESIGNED FOR THE ASSAY OF A 96 WELL PLATE (100 ASSAY POINTS). YOU MAY USE THIS KIT TO ASSAY A SINGLE 384-, 96-, 24-, OR 12-WELL PLATE OF HUMAN ADIPOCYTES. YOU MUST THEN TRANSFER THE CONDITIONED ASSAY BUFFER TO A 96 WELL FORMAT TO COMPLETE THE ASSAY.**

## B. LIPOLYSIS PROCEDURE

1. Make a stock solution using the appropriate vehicle for your test compounds. Dilute your vehicle and compound solutions to their final concentration in Assay Buffer (100 ml is available). NOTE: if desired, maintain a constant concentration of solvent by preparing all compound dilutions in the highest concentration of that solvent. Dilute the controls in assay buffer. Prepare all vehicles as appropriate for your compounds, 0.1% DMSO has been included as the vehicle for the positive controls. Include the Assay Buffer alone as a vehicle control. PLEASE NOTE: ZEN-BIO DOES NOT RECOMMEND THE USE OF SOLVENTS AT CONCENTRATIONS ABOVE 0.1%.


**Table 3. Lipolysis Assay Volumes**

FORMAT	REMOVE MEDIA TO GENTLY ADD WASH BUFFER		CHANGE WASH BUFFER		CHANGE WASH BUFFER TO ASSAY BUFFER	
	OUT	IN	OUT	IN	OUT	IN
384 well	20 µl/ well	30µl/ well	30µl/ well	30µl/ well	All media	20 µl/ well
96 well	120 µl/ well	200µl/ well	200µl/ well	200µl/ well	All media	150 µl/ well
48 well	400µl/ well	500µl/ well	500µl/ well	500 µl/ well	All media	250 µl/ well
24 well	0.8 ml/well	2.0 ml/well	0.6 ml/well	0.8 ml/well	All media	500 µl/ well
12 well	1.5 ml/well	2.0 ml/well	1.2 ml/well	1.6 ml/well	All media	1.0 ml/well

2. Remove Adipocyte Maintenance medium from each well. Gently add Wash Buffer to all wells. Remove some of the media and Wash Buffer from each well and replace with more Wash Buffer. See Table 3 for volumes.
3. Remove all the media and Wash Buffer from the cells from triplicate wells. Treat the cells with 150 µl of the test compounds resuspended in Assay Buffer three (3) wells at a time. [NOTE: for formats other than 96 wells, see column “CHANGE WASH BUFFER TO ASSAY BUFFER” in Table 3 for correct volume]. Treat with the diluted Isoproterenol or optionally, IBMX (for treatments 5-24 hours), as positive control. Use the Assay Buffer alone as one of the vehicle controls. Please be sure to include both the vehicle provided in the kit and your vehicle (if your test compounds are not dissolved in DMSO). The assay should be performed in triplicate.
4. OPTION: to determine if the compound alone reacts with the Glycerol Reagent A, prepare a fresh 96 well plate (not included in kit) containing 50 µl of the compound dilution. This plate can be incubated at 37°C with the treated cells. When performing the assay, add 50 µl of Glycerol Reagent A following the instructions in Steps 10 and 11.

5. Incubate the plates at 37°C-humidified incubator for 3 hours (for time course experiments the longest time point is usually 24 hours).
6. One hour prior to the assay, prepare the glycerol standards as follows:

Briefly spin down the contents of the glycerol standard tube before reconstitution. Pipette 400  $\mu$ l of Wash Buffer into the 1 mM glycerol standard tube provided and mix well by vortexing. This produces a diluted stock glycerol standard of 200  $\mu$ M. Pipette 250  $\mu$ l of wash buffer into 6 tubes (not provided). Using the newly diluted stock glycerol solution, prepare a dilution series as depicted below. Mix each new dilution thoroughly before proceeding to the next. The 200  $\mu$ M stock dilution serves as the highest standard, and the wash buffer serves as the zero standard.

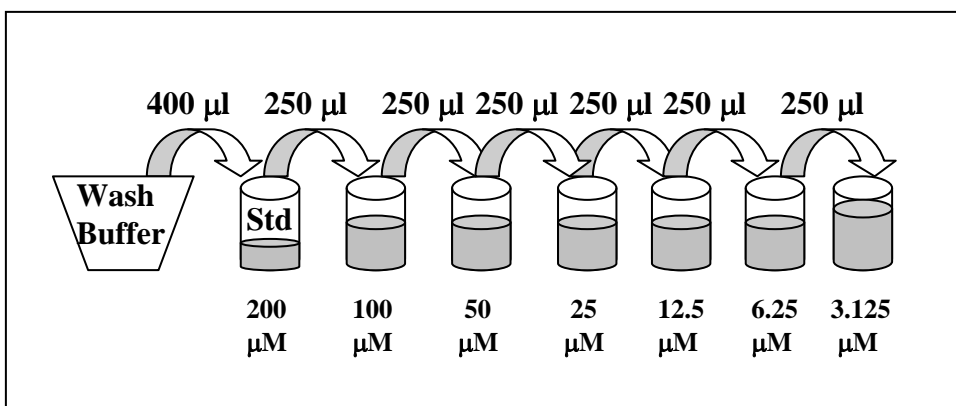

**Note: The above dilution series generates enough volume to perform the standard curve in duplicate. If you wish to perform the standard curve in duplicate, please note that eight fewer data points can be assayed with this kit.**

7. Also at this time prepare the Glycerol Reagent A by adding 11.0 ml room temperature deionized water per bottle and gently invert. DO NOT VORTEX! Use a pipet to ensure that the powder is completely dissolved. If using a Reagent A solution previously prepared and stored at 2-8°C, also bring to room temperature. Make sure there is enough Reagent A from one solution to treat all the points in the assay. It may be necessary to combine solutions. Store in a light protected bottle. Reconstituted Glycerol Reagent A is stable for 60 days refrigerated (2-8°C); store any remaining solution refrigerated (2-8°C).
8. At the end of the incubation, 100  $\mu$ l of the conditioned media is removed and transferred to the corresponding well of a blank 96 well plate. [This is most easily accomplished using a multi-channel pipet for 96 and 384 well formats] Add 100  $\mu$ l of each glycerol standard to any remaining empty wells in one of the blank 96 well assay plates.

9. Add the reconstituted Glycerol Reagent A solution to one of the disposable trays provided in the kit. Add 100  $\mu\text{L}$  of Reagent A to each well of the 96 well assay plates containing samples. Gently, pipet up and down once to mix. Pop the bubbles using a large gauge needle or a clean pipet tip. The plate is then incubated at 25°C (room temperature) for 15 minutes.
10. The optical density of each well is then measured at 540 nm.


## GLYCEROL STANDARD CURVE

Generate standard curve: see example below

**[DO NOT use this standard curve to generate your data. This is an example.]**

Subtract the OD value of the 0  $\mu\text{M}$  standard from all OD values including the standard curve.

$\mu\text{M}$ glycerol	OD	OD	OD- blank	OD- blank	Avg OD- blank
0	0.044	0.041			0.043
3.125	0.054	0.053	0.012	0.011	0.011
6.25	0.062	0.063	0.020	0.021	0.020
12.5	0.083	0.084	0.041	0.042	0.041
25	0.126	0.125	0.084	0.083	0.083
50	0.205	0.208	0.163	0.166	0.164
100	0.372	0.374	0.330	0.332	0.331
200	0.698	0.697	0.656	0.655	0.655

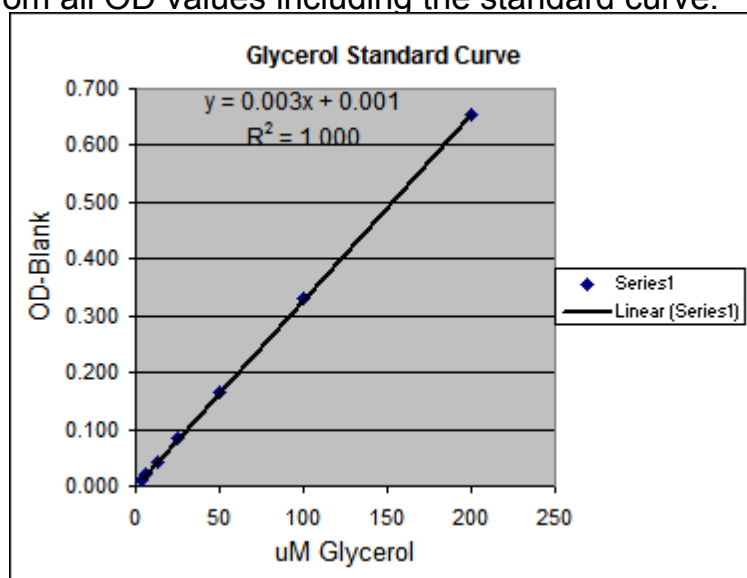

Slope	0.003
Intercept	0.001
$R^2$	1.000

y = observed O.D. minus the blank

x = concentration of glycerol in  $\mu\text{M}$

To calculate x for each y, (i.e. to change the observed O.D. into glycerol concentration) use the following equation:

$y = (\text{slope}) \times (x) + \text{intercept}$

$y = mx + b$  so  $x = (y - b)/m$

$x = (y - (0.001))/0.003$  where 0.003 = slope of the line and 0.001 = y intercept. Be careful to enter the proper sign for the y intercept value as it may be a negative number.



Any OD values greater than the highest standard (200  $\mu$ M) ☐☐☐ should be suspect. The compound should be re-assayed using a lower dose of the compound at treatment OR a dilute solution of the condition medium at the time of the assay.

**The  $R^2$  value should be equal or greater then 0.98 for the standard curve to be valid. Any  $R^2$  values below 0.98, must have the standard curve run again.**

Data are expressed as  $\mu$ M glycerol released.

OPTION: express data as Fold induction over appropriate vehicle

$$\text{Fold induction} = \frac{\mu\text{M glycerol SAMPLE}}{\mu\text{M glycerol VEHICLE}}$$

## FREQUENTLY ASKED QUESTIONS

---

- 1. When do I need to use the IBMX positive control?** If you use the 3-5 hour incubation described in this manual, you will not need to use the IBMX as your positive control. The IBMX positive control is designed for treatments ranging from 5-24 hours. The IBMX alternate control may be used in addition to the Isoproterenol positive control if your treatment time will exceed 5 hours.
- 2. Can I buy the reagents separately?** The Glycerol Standard, cat# LIP-GLYSTAN and Glycerol Reagent A, cat# RGTA-10 are sold separately. Assay Buffer is not sold separately. A REAGENTS ONLY kit is available cat# LIP-1-NC. Contact ZenBio to order additional cells or media.
- 3. I need to know the concentration of the BSA in the Assay Buffer?** ZenBio, Inc does not provide the concentrations of the components of our media and buffers. If knowledge of the BSA concentration is critical to your experiment, you may order Assay Buffer WITHOUT BSA for no additional charge. Please note it on your order.
- 4. I have more samples plus standards to run than can fit on 1 96 well plate. Can I compare data obtained from multiple plates?** The lipolysis kit is designed for the assay of a single plate. You may purchase 2 kits of the same lot number. You may then use one plate that includes the blank, vehicle(s), and positive and negative controls. The second plate may then be used for the remainder of your samples assayed. In order to obtain comparable data, both plates must be assayed on the same day using kits and cells from the same lot number. An additional blank assay plate is provided for the assay of glycerol standards.
- 5. I do not have time to pop the bubbles and read the plate. Can I freeze the conditioned media in one of the assay plates provided with the kit? How long can I store the samples before I complete the assay?** Yes. The conditioned media can be immediately stored at  $-80^{\circ}\text{C}$  for a maximum of 7 days. Bring the conditioned media in the plate to room temperature BEFORE adding the Glycerol Reagent A and completing the assay.




APPENDIX A: PLATE LAYOUT

---

H	G	F	E	D	C	B	A	
								1
								2
								3
								4
								5
								6
								7
								8
								9
								10
								11
								12

# APPENDIX B: PROCEDURE FLOWCHART

## ON DAY OF ASSAY 96 WELL FORMAT

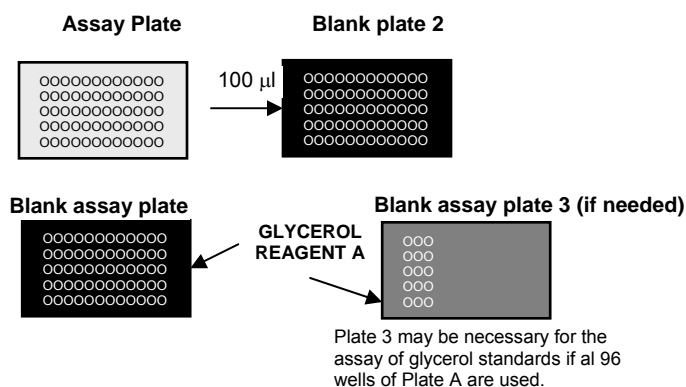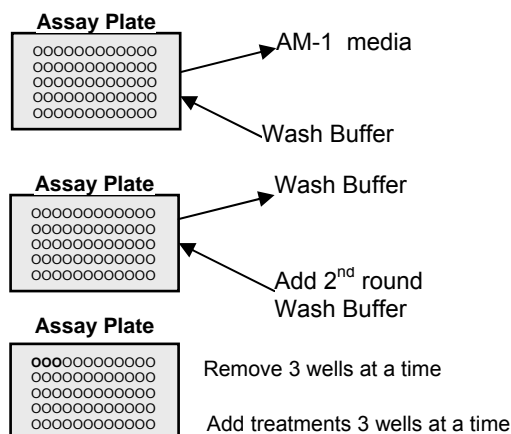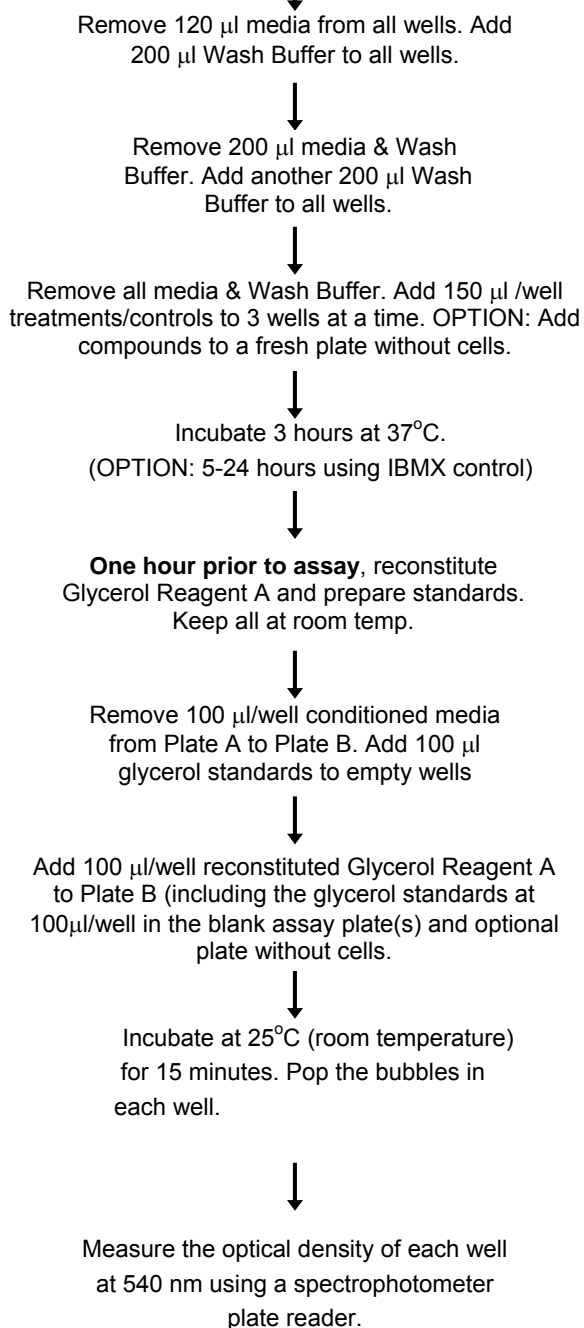

## REFERENCES

---

1. Arner P (1996) *Diabetes Rev* 4(4):450-463.
2. Botton LM & Green A. *Diabetes* (1999) 48:1691-1697
3. Brasaemle DL, Dolios G, Shapiro L, Wang R. (2004) *J Biol Chem* 279(45): 46835-42.
4. Cooper DMF, Schlegel W, Lin MC, Rodbell M. (1979) *J Biol Chem* 254(18):8927-8931.
5. Dyck DJ *Can J Appl Physiol* (2000) 25(6):495-523.
6. Kordik CP & Reitz AB. *J Medicinal Chem* (1999) 42(2):181-201.
7. Rieusset J, Chambrier C, Bouzakri K, Dussere E, Auwerx J, Riou J-P, Laville M, Vidal H. *Diabetologia* (2001) 44:544-554.
8. Robidoux J, Martin TL, Collins S. (2004) *Ann Rev Chem* 253: 7570-7578.
9. Scriba D, Aprath-Husmann I, Blum WF, Hauner H. *Eur J Endocrinol* (2000) 143:439-445
10. Snyder PB *Emerging Therapeutic Targets* (1999) 3(4): 587-599.
10. Tansey JT, Sztalryd C, Hlavin EM, Kimmel AR, Londos C. (2004) *IUBMB Life* 56(7): 379-85.